

Phospholipid Assay Kit (Colorimetric/Fluorometric)

LS-K185-100 (100 Tests) • Store at -20°C



Introduction

Phospholipids are a class of lipids which constitute a major component of cell membranes and play important roles in signal transduction. Most phospholipids contain one diglyceride, a phosphate group, and one choline. This Method provides a simple, direct and high-throughput assay for measuring choline-containing phospholipids in biological samples. In this assay, phospholipids (such as lecithin, lysolecithin and sphingomyelin) are enzymatically hydrolyzed to choline which is determined using choline oxidase and a H₂O₂ specific dye. The optical density of the pink colored product at 570nm or fluorescence intensity (530/585 nm) is directly proportional to the phospholipid concentration in the sample.

Key Features

- Sensitive. Use 20 µL samples. Linear detection range: colorimetric assay 3 - 200 µM, fluorometric assay 0.6 - 20 µM phospholipid.

Applications

- Assays: phospholipid in biological samples such as serum and non-EDTA plasma.
- Drug Discovery/Pharmacology: effects of drugs on choline-containing phospholipid metabolism.

Components

Component	K185-100
	100 Tests
Assay Buffer	10 mL
Enzyme Mix	Dried
PLD Enzyme	120 µL
Dye Reagent	120 µL
Standard (2 mM phosphatidylcholine)	400 µL

Materials Not Supplied

Pipetting devices, centrifuge tubes, clear flat-bottom uncoated 96-well plates, optical density plate reader; black flat-bottom uncoated 96-well plates, fluorescence plate reader.

Storage

The kit is shipped on ice. Store all components at -20°C. Shelf life of six months after receipt.

FOR RESEARCH USE ONLY! Not for use in humans.

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121
www.LSBio.com • (206) 464-1554 • TechnicalSupport@LSBio.com

Phospholipid Assay Kit (Colorimetric/Fluorometric)

LS-K185-100 (100 Tests) • Store at -20°C



Assay Procedure

Colorimetric Procedure

Liquid samples such as serum and plasma can be assayed directly. Solid samples can be homogenized in the assay buffer.

Note: SH-containing reagents (e.g. β -mercaptoethanol, dithiothreitol, > 5 μ M), sodium azide, EDTA, and sodium dodecyl sulfate are known to interfere in this assay and should be avoided in sample preparation.

1. Equilibrate all components to room temperature. Briefly centrifuge the tubes before opening. Keep thawed tubes on ice during assay. Reconstitute Enzyme Mix with 120 μ L Assay Buffer. Reconstituted Enzyme Mix is stable for 1 month when stored at -20°C. Note: a yellow precipitate may form after thawing reconstituted Enzyme Mix. If a precipitate forms, pellet it by centrifuging for 2 min at 14000 rpm and use the clear supernatant.
2. Standards: mix 24 μ L 2 mM Standard with 216 μ L dH₂O (final 200 μ M). Dilute standard in dH₂O as follows.

No	200 μ M STD + H ₂ O	Vol (μ L)	Standard (μ M)
1	100 μ L + 0 μ L	100	200
2	60 μ L + 40 μ L	100	120
3	30 μ L + 70 μ L	100	60
4	0 μ L + 100 μ L	100	0

Transfer 20 μ L diluted standards into separate wells of a clear flat-bottom 96-well plate.

Samples: transfer 20 μ L of each sample into separate wells of the plate.

Note: if a sample is known to contain choline, prepare an extra sample blank well with 20 μ L of the sample.

3. Color reaction. Prepare enough Working Reagent by mixing, for each well, 85 μ L Assay Buffer, 1 μ L PLD Enzyme, 1 μ L Enzyme Mix and 1 μ L Dye Reagent. Add 80 μ L Working Reagent to each well. For samples that contain choline, prepare a blank control reagent with no PLD Enzyme (i.e., 85 μ L Assay Buffer, 1 μ L Enzyme Mix and 1 μ L Dye Reagent). Add 80 μ L of the Control Reagent to the Sample Blank well.

Tap plate to mix. Incubate 30 min at room temperature.

Note: if precipitation occurs with certain samples, carry out the reaction in centrifuge tubes. After the 30 min incubation, centrifuge 5 min at 14,000 rpm. Transfer the supernatant into the wells for OD reading.

4. Read optical density at 570 nm (550-585 nm).

Fluorometric Procedure

The fluorometric assay procedure is similar to the colorimetric procedure except that (1) 0, 6, 12 and 20 μ M phospholipid standards and (2) a black 96-well plate are used. Read fluorescence intensity at λ_{ex} = 530 nm and λ_{em} = 585 nm.

Note: if the calculated phospholipid concentration of a sample is higher than 200 μ M in the Colorimetric Assay or 20 μ M in the Fluorimetric Assay, dilute sample in 0.5% Triton X-100 and repeat the assay. Multiply result by the dilution factor n .

FOR RESEARCH USE ONLY! Not for use in humans.

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121

www.LSBio.com • (206) 464-1554 • TechnicalSupport@LSBio.com

Phospholipid Assay Kit (Colorimetric/Fluorometric)

LS-K185-100 (100 Tests) • Store at -20°C




Calculations

Subtract blank value (#4) from the standard values and plot the ΔOD or ΔF against standard concentrations. Determine the slope and calculate the phospholipid concentration of Sample,

$$[\text{Phospholipid}] = \frac{R_{\text{SAMPLE}} - R_{\text{BLANK}}}{\text{Slope } (\mu\text{M}^{-1})} \times n \quad (\mu\text{M})$$

R_{SAMPLE} and R_{BLANK} are optical density or fluorescence intensity readings of the Sample and H₂O Blank (or Sample Blank if sample contains choline), respectively. n is the sample dilution factor.

Sample Data

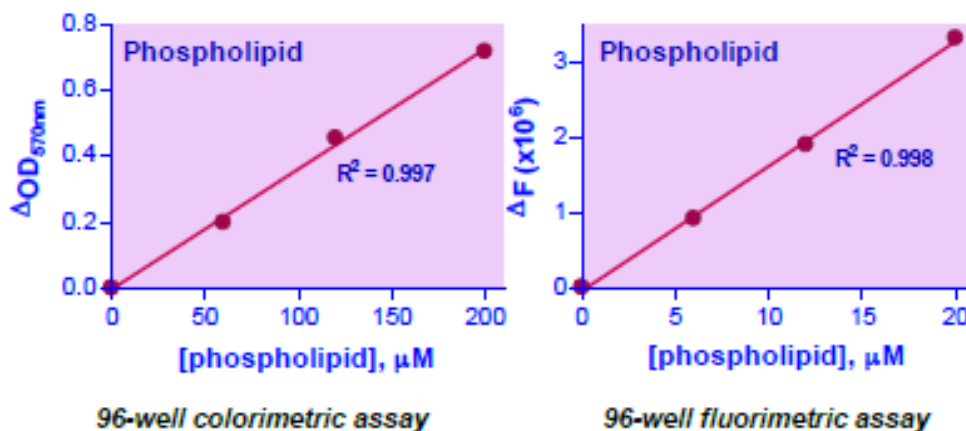

Version: V.08.09.2018

FOR RESEARCH USE ONLY! Not for use in humans.

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121

www.LSBio.com • (206) 464-1554 • TechnicalSupport@LSBio.com