

# D-Mannitol Assay Kit (Colorimetric)

LS-K163-100 (100 Tests) • Store at -20°C



---

## Introduction

D-MANNITOL (C<sub>6</sub>H<sub>14</sub>O<sub>6</sub>) is a sugar alcohol used in dietary supplement, sweetener, intestinal permeability test for leaky gut, etc. It also serves as a coating for hard candies, dried fruits, and chewing gums due to its low ability to attract and hold water molecules. In addition, it is an osmoprotectant for plants and is used clinically in osmotherapy to reduce intracranial pressure.

LSBio's D-mannitol assay kit is based on mannitol dehydrogenase catalyzed oxidation of D-mannitol, which generates D-fructose and NADH that reduces a formazan (MTT) dye. The intensity of product color, measured at 565 nm is directly proportional to D-mannitol concentration in the sample.

## Key Features

- Fast and sensitive. Use of 20 µL sample. Linear detection range 0.007 to 3 mM mannitol in 96-well plate assay.
- Convenient. The procedure involves adding a single working reagent, and reading the absorbance after 30 minutes. Room temperature assay. No 37°C heater is needed.
- High-throughput. "Add-mix-read" type assay. Can be readily automated as a high-throughput 96-well plate assay for thousands of samples per day.

## Applications

- Direct Assays: mannitol in food, beverage, agricultural products, and biological samples such as urine and serum.

## Components

| Component                    | K163-100  |
|------------------------------|-----------|
|                              | 100 Tests |
| Assay Buffer                 | 10 mL     |
| Enzyme                       | 120 µL    |
| Standard (~20 mM D-Mannitol) | 0.5 mL    |

## Materials Not Supplied

Pipetting devices, centrifuge tubes, clear flat-bottom 96-well plates (e.g. VWR cat# 82050-760), and plate reader.

## Storage

The kit is shipped on ice. Store all kit components at -20 °C.

---

**FOR RESEARCH USE ONLY! Not for use in humans.**

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121

[www.LSBio.com](http://www.LSBio.com) • (206) 464-1554 • [TechnicalSupport@LSBio.com](mailto:TechnicalSupport@LSBio.com)

# D-Mannitol Assay Kit (Colorimetric)

LS-K163-100 (100 Tests) • Store at -20°C



## Assay Procedure

### Sample Preparation

Clear and slightly colored samples can be assayed directly. It is prudent to test several dilutions to determine an optimal dilution factor  $n$ .

*Solid* samples can be homogenized in distilled water followed by filtration or centrifugation (e.g. 5-10 min 14,000 rpm).

*Beverage* samples can be assayed directly. Check the pH of the sample and adjust to 8-9 with NaOH or HCl if necessary. Samples containing carbon dioxide should be degassed by gentle stirring prior assay.

*Biological fluid samples* (e.g. urine & serum) can be assayed directly. Appropriate dilution in distilled water may be required.

### Procedure using 96-well plate

1. Standards. Prepare 200  $\mu\text{L}$  3 mM Premix by mixing 30  $\mu\text{L}$  of the Standard (20 mM) and 170  $\mu\text{L}$  distilled water. Dilute standards in 1.5-mL centrifuge tubes as described in the Table.

| No | Premix + H <sub>2</sub> O           | D-Mannitol (mM) |
|----|-------------------------------------|-----------------|
| 1  | 100 $\mu\text{L}$ + 0 $\mu\text{L}$ | 3.0             |
| 2  | 60 $\mu\text{L}$ + 40 $\mu\text{L}$ | 1.8             |
| 3  | 30 $\mu\text{L}$ + 70 $\mu\text{L}$ | 0.9             |
| 4  | 0 $\mu\text{L}$ + 100 $\mu\text{L}$ | 0               |

2. Transfer 20  $\mu\text{L}$  standards into separate wells of a clear, flat-bottom 96-well plate. Transfer 20  $\mu\text{L}$  of each sample into two separate wells, one serving as a sample blank well (OD<sub>BLANK</sub>) and one as a sample well (OD<sub>SAMPLE</sub>).
3. Prepare sufficient Working Reagent (WR) for all sample and standard wells by mixing, for each well: 85  $\mu\text{L}$  Assay Buffer plus 1  $\mu\text{L}$  Enzyme. Add 80  $\mu\text{L}$  WR to the four Standards and the Sample Wells.

Add 80  $\mu\text{L}$  Assay Buffer (i.e. no Enzyme) to the Sample Blank Wells. Tap plate to mix briefly and thoroughly. Incubate 30 minutes at room temperature.

4. Read optical density at 565 nm (520-600 nm).

### Calculations

Subtract the blank value (#4) from the standard values and plot the DOD against standard concentrations. Determine the slope and calculate the mannitol concentration of Sample,

$$[\text{D-Mannitol}] = \frac{\text{OD}_{\text{SAMPLE}} - \text{OD}_{\text{BLANK}}}{\text{Slope (mM}^{-1})} \times n \text{ (mM)}$$

OD<sub>SAMPLE</sub> and OD<sub>BLANK</sub> are optical density readings of the Sample and Sample Blank, respectively.  $n$  is the sample dilution factor.

Note: if the sample OD value is higher than OD for the 3 mM mannitol standard, dilute sample in water and repeat the assay. Multiply the results by the dilution factor.

Conversions: 1 mM D-mannitol equals 18.2 mg/dL, or 182 ppm.

**FOR RESEARCH USE ONLY! Not for use in humans.**

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121

[www.LSBio.com](http://www.LSBio.com) • (206) 464-1554 • [TechnicalSupport@LSBio.com](mailto:TechnicalSupport@LSBio.com)


# D-Mannitol Assay Kit (Colorimetric)

LS-K163-100 (100 Tests) • Store at -20°C



---

## Sample Data

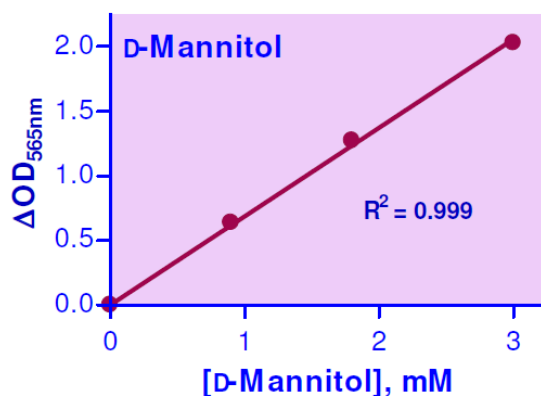

Standard Curve in 96-well plate assay in water

Version: V.08.09.2018

---

**FOR RESEARCH USE ONLY! Not for use in humans.**

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121  
[www.LSBio.com](http://www.LSBio.com) • (206) 464-1554 • [TechnicalSupport@LSBio.com](mailto:TechnicalSupport@LSBio.com)