

# **LSBio™ Mouse CSF2 / GM-CSF ELISA Kit**

**Catalog No. LS-F607**

## **User Manual**

**Please Read the Manual Carefully  
Before Starting your Experiment**



**LSBio**

For research use only. Not approved for use in humans or for clinical diagnosis.

# CONTENTS

# PAGE

|                                       |    |
|---------------------------------------|----|
| Introduction.....                     | 3  |
| Assay Principles.....                 | 4  |
| Assay Format.....                     | 5  |
| Assay Restrictions.....               | 6  |
| Materials Included.....               | 6  |
| Additional Materials Required.....    | 7  |
| Health and Safety Precautions.....    | 7  |
| Storage Information.....              | 8  |
| Sample Preparation and Storage.....   | 9  |
| Sample Experiment Layout.....         | 10 |
| Immunoassay Protocol.....             | 11 |
| Summarized Protocol.....              | 16 |
| Sensitivity.....                      | 17 |
| Cross Reactivity and Specificity..... | 17 |

## INTRODUCTION

Murine GM-CSF, also known as Granulocyte-Macrophage Colony-Stimulating Factor, is a 141 amino acid cytokine protein encoded by the *Csf2* gene located at chromosome 11. After initial synthesis and translocation, the 17 residue signal sequence is cleaved from the N-terminal region, allowing the 124 residue GM-CSF peptide to fold properly into its mature form. Belonging to the GM-CSF family, GM-CSF, a monomeric cytokine, essentially stimulates the growth and differentiation of hematopoietic precursor cells from various lineages, including granulocytes, macrophages, eosinophils and erythrocytes. It is able to be modified via O-linked and N-linked glycosylation.


*Source: Entrez Gene: Csf2 colony stimulating factor 2 (granulocyte-macrophage) [Mus musculus]; Swiss-Prot: P01587*

## ASSAY PRINCIPLES

The LSBio™ Murine GM-CSF ELISA Kit contains the components necessary for quantitative determination of natural or recombinant Murine GM-CSF concentrations within any experimental sample including cell lysates, serum and plasma. This particular immunoassay utilizes the quantitative technique of a “Sandwich” Enzyme-Linked Immunosorbent Assay (ELISA) where the target protein (antigen) is bound in a “sandwich” format by the primary capture antibodies coated to each well-bottom and the secondary detection antibodies added subsequently by the investigator. The capture antibodies coated to the bottom of each well are specific for a particular epitope on Murine GM-CSF while the user-added detection antibodies bind to epitopes on the captured target protein. Amid each step of the procedure, a series of wash steps must be performed to ensure the elimination of non-specific binding between proteins to other proteins or to the solid phase. After incubation and “sandwiching” of the target antigen, a peroxidase enzyme is conjugated to the constant heavy chain of the secondary antibody (either covalently or via Avidin/Streptavidin-Biotin interactions), allowing for a colorimetric reaction to ensue upon substrate addition. When the substrate TMB (3, 3', 5, 5'-Tetramethylbenzidine) is added, the reaction catalyzed by peroxidase yields a blue color that is representative of the antigen concentration. Upon sufficient color development, the reaction can be terminated through addition of Stop Solution (2 N Sulfuric Acid) where the color of the solution will turn yellow. The absorbance of each well can then be read by a spectrophotometer, allowing for generation of a standard curve and subsequent determination of protein concentration.


# ASSAY FORMAT

  
**Capture Antibody**

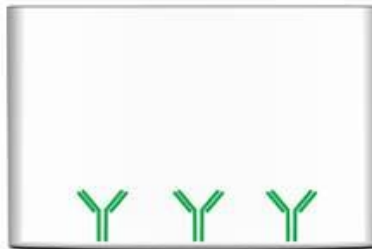


**Capture antibodies specific for the target are coated to the plate. Additional binding sites on the plate are blocked.**

  
**Target Antigen**

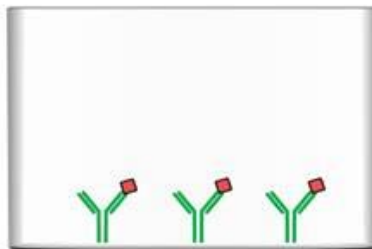


**Target antigen present in standard or sample is bound by capture antibodies on the solid-phase.**

  
**Biotinylated Detection Antibody**

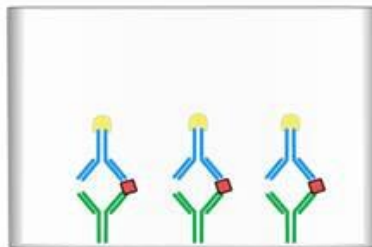


**Biotinylated detection antibodies specific for the target are added to bind another epitope on the target antigen.**

  
**Streptavidin-HRP**

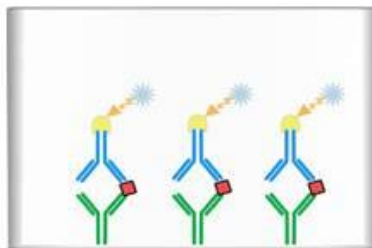

**Streptavidin-HRP attaches to detection antibody via high affinity streptavidin-biotin interaction.**

  
**Unreacted TMB**

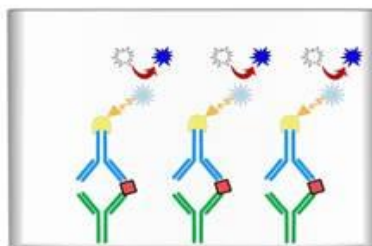

**TMB substrate is converted to the blue TMB diimine via the HRP enzyme. Upon addition of acid, the reaction terminates and the wells can be read at 450 nm.**

  
**Blue TMB Diimine Product**

## ASSAY RESTRICTIONS

- This ELISA kit is intended for research purposes only, NOT diagnostic or clinical procedures of any kind.
- Materials included in this kit should NOT be used past the expiration date on the kit label.
- Reagents or substrates included in this kit should NOT be mixed or substituted with reagents or substrates from any other kits.
- Variations in pipetting technique, washing technique, operator laboratory technique, kit age, incubation time or temperature may cause differences in binding affinity of the materials provided.
- The assay is designed to eliminate interference and background by other cellular macromolecules or factors present within any biological samples. However, the possibility of background noise cannot be fully excluded until all factors have been tested using the assay kit.

## MATERIALS INCLUDED

| Component                              | Quantity Per Plate      | Container |
|----------------------------------------|-------------------------|-----------|
| Microstrips Coated w/ Capture Antibody | 12 x 8-Well Microstrips | -         |
| Protein Standard                       | Lyophilized             | Red       |
| Biotinylated Detection Antibody        | Lyophilized             | Yellow    |
| 400x Streptavidin-HRP                  | 30 $\mu$ l              | Blue      |
| Wash Buffer (15x)                      | 50 ml                   | Clear     |
| Assay Diluent                          | 50 ml                   | Clear     |
| Ready-to-Use Substrate                 | 12 ml                   | Brown     |
| Stop Solution                          | 12 ml                   | Clear     |
| Adhesive Plate Sealers                 | 4 Sheets                | -         |
| Technical Manual                       | 1 Manual                | -         |

## ADDITIONAL MATERIALS REQUIRED

The following materials and/or equipment are NOT provided in this kit but are necessary to successfully conduct the experiment:

- Microplate reader able to measure absorbance at 450 nm (with correction wavelength set to 540 nm or 570 nm)
- Micropipettes with capability of measuring volumes ranging from 1  $\mu$ l to 1 ml
- Deionized or sterile water
- Squirt bottle, manifold dispenser, multichannel pipette reservoir or automated microplate washer
- Graph paper or computer software capable of generating or displaying logarithmic functions
- Absorbent paper or vacuum aspirator
- Test tubes or microfuge tubes capable of storing  $\geq 1$  ml
- Bench-top centrifuge (optional)
- Bench-top vortex (optional)
- Orbital shaker (optional)

## HEALTH AND SAFETY PRECAUTIONS

- Reagents provided in this kit may be harmful if ingested, inhaled or absorbed through the skin. Please carefully review the MSDS for each reagent before conducting the experiment.
- Stop Solution contains 2 N Sulfuric Acid ( $\text{H}_2\text{SO}_4$ ) and is an extremely corrosive agent. Please wear proper eye, hand and face protection when handling this material. When the experiment is finished, be sure to rinse the plate with copious amounts of running water to dilute the Stop Solution prior to disposing the plate.

## STORAGE INFORMATION

**Note:** If used frequently, reagents may be stored at 4°C.

**Unopened Kits:** Store at 4°C for 6 months.

| Component                                 | Storage Time                                    | Storage Information |
|-------------------------------------------|-------------------------------------------------|---------------------|
| Microstrips Coated w/<br>Capture Antibody | 6 Months                                        | 4°C                 |
| 400x Streptavidin-HRP                     |                                                 |                     |
| Wash Buffer (15x)                         |                                                 |                     |
| Assay Diluent                             |                                                 |                     |
| Ready-to-Use Substrate                    |                                                 |                     |
| Stop Solution                             |                                                 |                     |
| Protein Standard                          | Lyophilized: 6 Months<br>Reconstituted: 1 Month | 4°C                 |
| Biotinylated Detection<br>Antibody        |                                                 |                     |
| Adhesive Plate Sealers                    | -                                               | -                   |
| Technical Manual                          | -                                               | -                   |

# **SAMPLE PREPARATION AND STORAGE**

**Levels of Murine GM-CSF may vary between samples. Optimal dilution factors for every sample must be determined by the investigator.**

## ***Cell Supernatants***

Remove large cell components via centrifugation and perform the assay. Cell lysates and supernatants require a dilution using Assay Diluent 1TD. A serial dilution may be performed to determine a suitable dilution factor for the sample.

## ***Serum***

Allow samples to clot in a serum separator tube (SST) for 30 minutes. After sufficient clotting, centrifuge at 1000 x g for 15 minutes and remove serum from SST in preparation for the assay. A serial dilution may be performed to determine a suitable dilution factor for the sample. For serum sample dilutions refer to Serum and Plasma Sample Dilution Protocol.

## ***Plasma***

Use heparin, citrate or EDTA as an anticoagulant to gather plasma from original biological sample. After collection of the plasma, centrifuge for 15 minutes at 1000 x g. This step must be performed within 30 minutes of plasma collection. A serial dilution may be performed to determine a suitable dilution factor for the sample. For plasma sample dilutions refer to Serum and Plasma Sample Dilution Protocol.

**If samples are to be used within 24 hours, aliquot and store at 4°C. If samples are to be used over a long period of time, aliquot and store between -20°C and -80°C, depending on the duration of storage.**

**Samples containing a visible precipitate or pellet must be clarified prior to use in the assay.**

**Avoid repeated freeze/thaw cycles to prevent loss of biological activity of proteins in experimental samples.**

### ***Serum and Plasma Sample Dilution Protocol***

- a. Dilute the serum or plasma samples with PBS supplemented with 10-50% animal serum (Serum/Plasma Diluent).
- b. Reconstitute and dilute the Protein Standards using the Serum/Plasma Diluent, instead of Assay Diluent 1TD, so it reflects the environment of the samples being measured.
- c. Reconstitute/dilute the Biotin-Conjugated Detection Antibody in Assay Diluent 1TD and dilute the Streptavidin-HRP in Assay Diluent 1TD. Do not use the Serum/Plasma Diluent to reconstitute or dilute the Detection Antibody or Streptavidin-HRP.


## SAMPLE EXPERIMENT LAYOUT

|   | 1                        | 2                        | 3                        | 4      | 5      | 6      |
|---|--------------------------|--------------------------|--------------------------|--------|--------|--------|
| A | Standard<br>(High Point) | Standard<br>(High Point) | Standard<br>(High Point) | Sample | Sample | Sample |
| B | Standard<br>(1:2)        | Standard<br>(1:2)        | Standard<br>(1:2)        | Sample | Sample | Sample |
| C | Standard<br>(1:4)        | Standard<br>(1:4)        | Standard<br>(1:4)        | Sample | Sample | Sample |
| D | Standard<br>(1:8)        | Standard<br>(1:8)        | Standard<br>(1:8)        | Sample | Sample | Sample |
| E | Standard<br>(1:16)       | Standard<br>(1:16)       | Standard<br>(1:16)       | Sample | Sample | Sample |
| F | Standard<br>(1:32)       | Standard<br>(1:32)       | Standard<br>(1:32)       | Sample | Sample | Sample |
| G | Standard<br>(1:64)       | Standard<br>(1:64)       | Standard<br>(1:64)       | Sample | Sample | Sample |
| H | Negative<br>Control      | Negative<br>Control      | Negative<br>Control      | Sample | Sample | Sample |

## REAGENT PREPARATION

All provided solutions should be at ambient temperature prior to use. **We recommend performing the assay in duplicate.** Reagents provided are enough to assay 96 wells and it is recommended to only prepare as much needed on the day of the experiment. All incubation steps should be performed on an orbital shaker to equilibrate solutions when added to the microplate wells.

1. Dilute the 15x Wash Buffer to 1x Wash Buffer using 14 volumes of ddH<sub>2</sub>O and 1 volume of 15x Wash Buffer.
2. Reconstitute Detection Antibody with 100 µl of ddH<sub>2</sub>O for a concentration of 100x. Mix gently and dilute to 1x prior to use.
3. Reconstitute Protein Standard with 83 µl of ddH<sub>2</sub>O for a concentration of 250 ng/mL. Mix gently and dilute to the working range of the kit, 32-4000 pg/ml.
  - a. Dilute Protein Standard with the same reagents used with Serum/Plasma samples. **OR.**
  - b. Dilute Protein Standard with Assay Diluent 1TD when experimenting with Cell Supernatant samples.

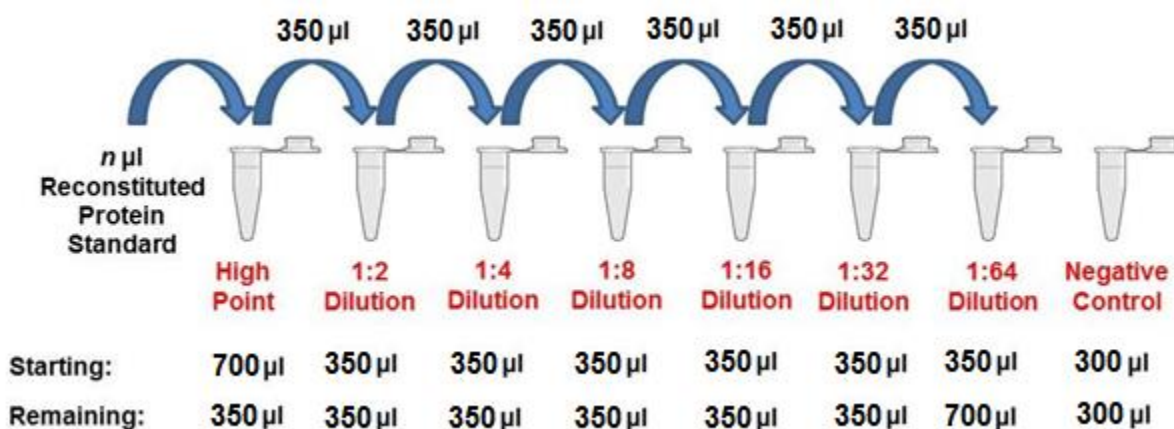

4. Mix the 400x Streptavidin-HRP (SAV-HRP) gently. Dilute to 1x using Assay Diluent 1TD.
5. Stop Solution and Ready to Use Substrate are ready to use and do not need dilution.

## ASSAY PROCEDURE

1. Prepare all reagents to working concentrations, standards to desired range, and samples to appropriate dilution factors.
2. Remove desired number of capture antibody coated strips for experiment and place remaining strips back into dry pouch with desiccant for 4°C storage.
3. Add 100 µl of Standards/ Samples to each well and incubate on orbital shaker at room temperature (RT) for 2 hrs.
4. Aspirate the solution and add 300 µl of 1x Wash Buffer to each well being used and gently shake for 2-3 mins on an orbital shaker. Repeat this process 3 times. After the last wash ensure no liquid remains by inverting the plate and tapping it against clean paper towels.
5. Add 100 µl of 1x Detection Antibody to each well and incubate for 2 hrs. on an orbital shaker at RT
6. Repeat step 4.
7. Add 100 µl of 1x SAV-HRP to each well and incubate for 30 mins on an orbital shaker at RT
8. Repeat step 4.
9. Add 100 µl of Ready to use Substrate to each well, cover plate from light, and incubate for 10-20 mins on an orbital shaker at RT. Monitor color development as the buffer used to dilute Serum and Plasma samples can effect rate of development.
10. Add 100 µl of Stop Solution to each well and read at 450 nm.


## DATA ANALYSIS

Average the duplicate or triplicate readings for each standard, control and sample and subtract the average zero standard optical density.

Generate a standard curve by using Microsoft Excel or other computer software capable of establishing a 4-Parameter Logistic (4-PL) curve fit. If using Excel or an alternative graphing tool, plot the average optical density values in absorbance units (y-axis) against the known standard concentrations in pg/ml (x-axis).

Only use the values in which a noticeable gradient can be established. Afterwards, generate a best fit curve or “trend-line” through the plotted points via regression analysis.

## TYPICAL DATA

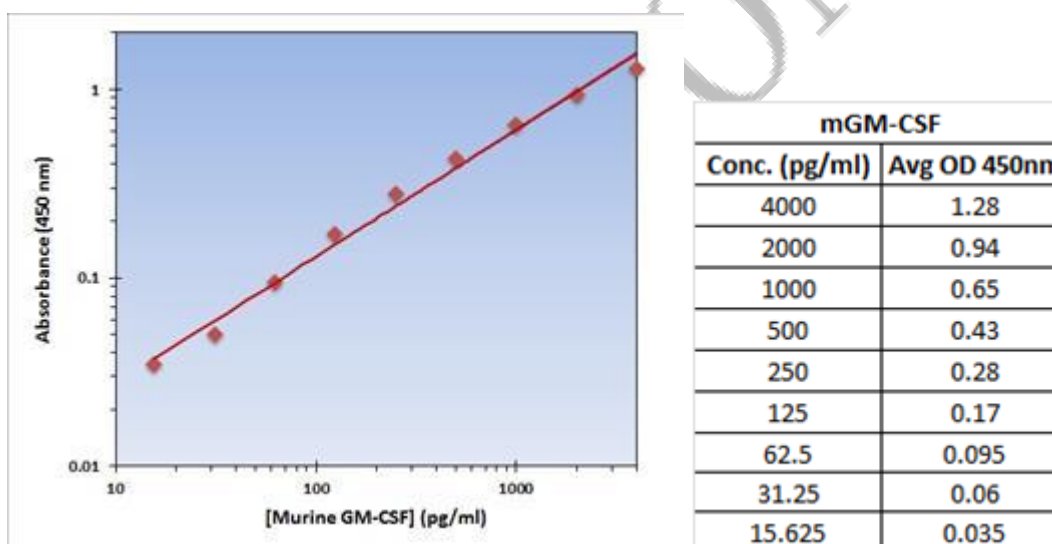

The data and subsequent graph were obtained after performing a sandwich ELISA for Murine GM-CSF. Each known sample concentration was assayed in triplicate.

The standard curves shown are for demonstration. A new curve must be generated for each experiment.

## **SENSITIVITY**

The Murine GM-CSF ELISA Kit allows for the detection and quantification of endogenous levels of natural and/or recombinant proteins within the range of 32-4000 pg/ml.

## **CROSS REACTIVITY AND SPECIFICITY**

The OmniKine™ Murine GM-CSF ELISA is capable of recognizing both recombinant and naturally produced Murine GM-CSF proteins. The antigens listed below were tested at 50 ng/ml and did not exhibit significant cross reactivity or interference.

- Human: GM-CSF, IL-2, IL-3, IL-4, IL-5, IL-7
- Murine: IL-2, IL-3, IL-4, IL-9, IL-15
- Rat: IL-2, IL-3beta, IL-4

# SUMMARIZED PROTOCOL

Reconstitute Biotinylated Detection Antibody and Protein Standard and dilute the 15x Wash Buffer as specified.



Perform serial dilution of Protein Standard and prepare samples as desired. See sample preparation section for instructions to dilute serum and plasma samples.



Add 100ul of Protein Standard, sample or control to each well and incubate for 2 hours at room temperature.



Aspirate Protein Standards, samples or controls out and wash plate 4 times.



Dilute Biotinylated Detection Antibody as specified. Add 100ul to each well and incubate for 2 hours at room temperature.



Aspirate Biotinylated Detection Antibody out and wash plate 4 times.



Dilute 400x Streptavidin-HRP as specified. Add 100ul of 1x Streptavidin-HRP to each well and incubate at room temperature for 30 minutes.



Aspirate 1x Streptavidin-HRP out and wash plate 4 times.



Add 100ul of Ready-to-Use Substrate to each well and incubate at room temperature for color development.



Add 100ul of Stop Solution and read plate at 450nm.

**Important Note:** During shipment, small volumes of product will occasionally become entrapped in the seal of the product vial. We recommend briefly centrifuging the vial to dislodge any liquid in the container's cap prior to opening.

**Warning:** This reagent may contain sodium azide and sulfuric acid. The chemical, physical, and toxicological properties of these materials have not been thoroughly investigated. Standard Laboratory Practices should be followed. Avoid skin and eye contact, inhalation, and ingestion. Sodium azide forms hydrazoic acid under acidic conditions and may react with lead or copper plumbing to form highly explosive metal azides. On disposal, flush with large volumes of water to prevent accumulation.

**Returns, Refunds, Cancellations:** Any problems with LifeSpan products must be reported to LifeSpan within 10 days of product receipt. The customer must obtain written authorization from LifeSpan before returning items. To request that goods be returned, please contact LifeSpan Technical Support. If an error by LifeSpan BioSciences results in shipment of an incorrect order, LifeSpan will, at its option, either ship a replacement order at no charge, or credit the customer's account for the original product shipped in error. Returns and cancellations may be subject to a 30% restocking fee.

**Conditions & Warranty:** All LifeSpan products are intended for Research Use Only and are not for use in human therapeutic or diagnostic applications. The information supplied with each product is believed to be accurate, but no warranty or guarantee is offered for the products, because the ultimate conditions of use are beyond LifeSpan's control. The information supplied with each product is not to be construed as a recommendation to use this product in violation of any patent, and LifeSpan will not be held responsible for any infringement or other violation that may occur with the use of its products. Under no event will LifeSpan be responsible for any loss of profit or indirect consequential damage, including, but not limited to, personal injuries resulting from use of these products. LifeSpan's liability to any user of Products for damages that do not result from any fault of the user, will be limited to replacement of the Product(s) only, and in no event shall LifeSpan's liability exceed the actual price received by LifeSpan for the Product(s) at issue. LifeSpan shall not be liable for any indirect, special, incidental or consequential damages. LIFESPAN FURTHER DISCLAIMS ANY AND ALL EXPRESS AND IMPLIED OR STATUTORY WARRANTIES WITH RESPECT TO THE PRODUCTS, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE. LifeSpan disclaims any and all responsibility for any injury or damage which may be caused by the fault of the user.

**For research use only. Not approved for use in humans or for clinical diagnosis.**



[Technical.Support@LSBio.com](mailto:Technical.Support@LSBio.com)